

© 2019 IEEE. Personal use of this material is permitted. Permission from IEEE must be obtained for all other uses, in any current or future media, including reprinting/republishing this material for advertising or promotional purposes, creating new collective works, for resale or redistribution to servers or lists, or reuse of any copyrighted component of this work in other works.

Cite as:

IEEE

M. Jafarzadeh, D. Hussey and Y. Tadesse, "Deep learning approach to control of prosthetic hands with electromyography signals", in *2019 IEEE International Symposium on Measurement and Control in Robotics (ISMCR)*, Houston, Texas, USA, 2019.

ACM

Jafarzadeh, M., Hussey, D. and Tadesse, Y., 2019. Deep learning approach to control of prosthetic hands with electromyography signals. In *2019 IEEE International Symposium on Measurement and Control in Robotics (ISMCR)*. IEEE.

MLA

Jafarzadeh, Mohsen et al. "Deep Learning Approach To Control Of Prosthetic Hands With Electromyography Signals". IEEE, *2019 IEEE International Symposium On Measurement And Control In Robotics (ISMCR)*. IEEE, 2019.

APA

Jafarzadeh, M., Hussey, D., & Tadesse, Y. (2019). Deep learning approach to control of prosthetic hands with electromyography signals. In *2019 IEEE International Symposium on Measurement and Control in Robotics (ISMCR)*. Houston, Texas, USA: IEEE.

Harvard

Jafarzadeh, M., Hussey, D. and Tadesse, Y. (2019). Deep learning approach to control of prosthetic hands with electromyography signals. In: *2019 IEEE International Symposium on Measurement and Control in Robotics (ISMCR)*. IEEE.

Vancouver

Jafarzadeh M, Hussey D, Tadesse Y. Deep learning approach to control of prosthetic hands with electromyography signals. 2019 IEEE International Symposium on Measurement and Control in Robotics (ISMCR). IEEE; 2019.

Chicago

Jafarzadeh, Mohsen, Daniel Curtiss Hussey, and Yonas Tadesse. 2019. "Deep Learning Approach To Control Of Prosthetic Hands With Electromyography Signals". In *2019 IEEE International Symposium On Measurement And Control In Robotics (ISMCR)*. IEEE.

BibTeX

```
@inbook{ jafarzadeh_hussey_tadesse_2019,[break] title={Deep learning approach to control of prosthetic hands with electromyography signals},[break] booktitle={2019 IEEE International Symposium on Measurement and Control in Robotics (ISMCR)},[break] publisher={IEEE},[break] author={Jafarzadeh, Mohsen and Hussey, Daniel Curtiss and Tadesse, Yonas},[break] year={2019}}
```

Deep learning approach to control of prosthetic hands with electromyography signals

Mohsen Jafarzadeh

Department of Electrical and Computer Engineering
The University of Texas at Dallas
Richardson, TX, USA
Mohsen.Jafarzadeh@utdallas.edu

Daniel Curtiss Hussey

Department of Electrical and Computer Engineering
The University of Texas at Dallas
Richardson, TX, USA
dch150330@utdallas.edu

Yonas Tadesse

Department of Mechanical Engineering
The University of Texas at Dallas
Richardson, TX, USA
Yonas.Tadesse@utdallas.edu

Abstract—Natural muscles provide mobility in response to nerve impulses. Electromyography (EMG) measures the electrical activity of muscles in response to a nerve's stimulation. In the past few decades, EMG signals have been used extensively in the identification of user intention to potentially control assistive devices such as smart wheelchairs, exoskeletons, and prosthetic devices. In the design of conventional assistive devices, developers optimize multiple subsystems independently. Feature extraction and feature description are essential subsystems of this approach. Therefore, researchers proposed various hand-crafted features to interpret EMG signals. However, the performance of conventional assistive devices is still unsatisfactory. In this paper, we propose a deep learning approach to control prosthetic hands with raw EMG signals. We use a novel deep convolutional neural network to eschew the feature-engineering step. Removing the feature extraction and feature description is an important step toward the paradigm of end-to-end optimization. Fine-tuning and personalization are additional advantages of our approach. The proposed approach is implemented in Python with TensorFlow deep learning library, and it runs in real-time in general-purpose graphics processing units of NVIDIA Jetson TX2 developer kit. Our results demonstrate the ability of our system to predict fingers position from raw EMG signals. We anticipate our EMG-based control system to be a starting point to design more sophisticated prosthetic hands. For example, a pressure measurement unit can be added to transfer the perception of the environment to the user. Furthermore, our system can be modified for other prosthetic devices.

Keywords—prosthetic hands, electromyography, EMG, deep learning, convolutional neural networks

I. INTRODUCTION

The human hand is a very important part, which enables humans to perform basic daily activities ranging from hand gestures to object manipulation. The loss of a hand is a severe mental and physical trauma for humans. It is estimated that there are approximately 94,000 upper limb amputees in Europe [1] and 41,000 upper limb amputees in the United States [2]. The World Health Organization estimates that there are about 40 million amputees in the world [3]. These numbers expected to grow further, due to an increased life expectancy and a corresponding higher incidence of diabetes and vascular diseases. High-performance prosthetic hands significantly improve the quality of life for upper-limb amputees. Passive prosthetic hands [4] are lightweight, robust, and quiet, but can only perform a limited subset of activities. Body-powered [5,6] prosthetic hands are neither intuitive to operate nor they adequately restore limb function. Therefore, developers have investigated externally-powered prosthetic hands for upper-limb amputees for more than a century [7,8]. Recent advances in prosthetic hands aid upper limb amputees to perform some activities that are difficult or impossible when wearing passive

devices, up to certain degrees. Control of these prosthetic hands is a key part of developing these devices. Although researchers have proposed many methods to control these hands, there is a huge gap between expected functionality and current state-of-the-art. Thus, control of prosthetic hands is still an open problem. There are several ways to command a prosthetic hand including but not limited to push-buttons, joystick, keyboard, vision, speech, electroencephalography (EEG), electromyography (EMG), and Electroneurography (ENG). Among these ways, electromyography is the most convenient for amputees. Therefore, in this paper, we only focus on controlling the prosthetic hand with electromyography.

Motor neurons transmit electrical signals that cause muscles to contract. Electromyography (EMG) measures muscle response or electrical activity in response to a nerve's stimulation of the muscle. In other words, an EMG electrode reads electric potential generated in the muscle fibers when they contract. There is a strong correlation between the electric potential in the muscle cell and the nerves cell [9]. There are two types of EMG sensors, surface electromyography (sEMG) and intramuscular EMG (imEMG). The imEMG sensors puncture the skin and directly contact to the muscles. Thus, imEMG sensors provide higher signal to noise ratios. Therefore, imEMG sensors are more accurate, especially for motions that involve multiple degrees of freedom of the human hand [10]. However, imEMG sensors are intrusive, painful, uncomfortable, and difficult to set up. Hence, we do not consider imEMG sensors in this paper. SEMG signals are measured with electrodes on the surface of the skin just above the target muscles. So, the sEMGs is a non-invasive technique. Surface EMG sensors typically use silver electrodes and contact with skins can be either wet (silver-chloride) or dry [11]. Wet sEMG sensors have higher signal to noise ratioa. However, the use of a gel is inconvenient for amputees. Here, we focus on the control of prosthetic hand using dry sEMG. For the rest of the paper, we use the term “EMG” word instead of “dry sEMG”.

Surface EMG signals have low signal to noise ratios. Therefore, these signals can be easily lost in the environmental noise. The maximum electric potential signal can be measured from sEMG sensors are typically 5 mV [12]. Therefore, in practice, these signals should be amplified (usually 500 to 2000 times) to be able to read with the market available analog to digital converters (ADC). Most EMG sensors in the market use bandpass filter range from 50 to 500 Hz. So, the ADC should be able to measure with the rate of 2000 or more samples per second. The 50 or 60 Hz is easily corrupted with noise because of the power-line in the cities [13]. Some researchers used band-stop filters for the EMG sensors to cancel the 50/60 Hz noise. However, the 50 and 60 Hz bands

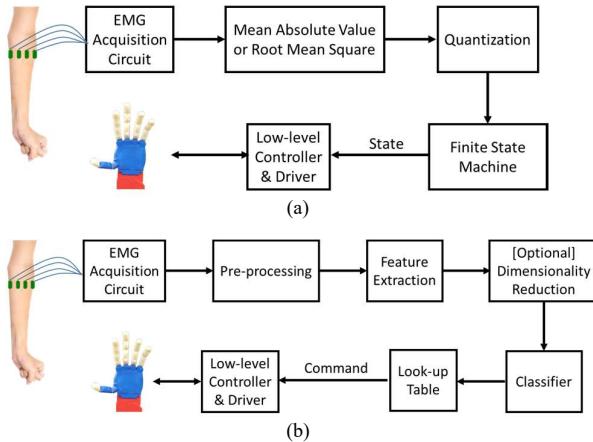


Fig. 1. Traditional approaches to control prosthetics hands with EMG signals (a) using finite-state machine and (b) using signal processing and pattern recognition methods.

contain very informative data about the EMG signal. Thus, a functional prosthetic hand should have a low-pass filter (10 Hz) in the power supply circuit to address the power-line noise. In short, designing a measurement circuit with low pass filters (10 Hz) for power-line, amplifiers (500 to 2000 times, typically 660 times), and a/few fast precision ADC (at least 2000 sample per second and preferably 16-bit noise-free resolution) is a key challenge in designing functional prosthetic hands with dry surface EMG sensors. An example of a circuit with 16-bit, 4000 samples per second, third-order Sigma-Delta ADC is demonstrated in [14]. Indeed, the EMG acquisition circuit must be addressed before designing any controller.

There are two traditional ways of controlling devices with EMG signals [15] as shown in Fig. 1. The first one is the quantization of mean absolute value (or root mean square) of EMG signals and using a finite state machine to determine the state of EMG and then use this state to control the device. Although this method is the easiest and most robust way to control the device with EMG, it limits the prosthetic hand to a few basic motions. The second one is using pattern recognition algorithms to classify EMG signals and then using a look-up table to convert the estimated class to a command. The second method typically consists of preprocessing, feature extraction, dimension reduction (feature description), classifier, and a look-up table. The pre-processing may include one or a combination of a high pass filter (10 to 50 Hz), a band-stop filter (50 or 60 Hz), a low pass filter (500 Hz), regression subtraction, spectrum interpolation, non-negative matrix factorization, etc. Feature extraction is the most important subsystem of this system. The feature should be robust to noise while it must discriminate the signals into different classes. A feature extraction system receive a processed EMG signal and computes a feature vector. Researchers have proposed many features [1,16] including but not limited to mean absolute value, integrated absolute value, variance, mean absolute value slope, root mean square, Willison amplitude, number of zero crossing, number of slope sign change, auto-regression coefficients, cepstral coefficient, mean of signal frequency, power spectral density, waveform length, min/max frequency ratio, short-time furrier transform, discrete wavelet transform, and wavelet packet transform. EMG pattern recognition systems typically use 8 or more EMG sensors and 5 or more features (for each sensor).

Therefore, the feature vector has a high dimension. Training of a system with a high dimension features requires a huge amount of data for training, validation, and testing. Therefore, researchers usually use feature description subsystem (dimension reduction techniques) such as principal component analysis (PCA), locality preserving projections (LPP), and neighborhood preserving embedding (NPE). Many EMG classifiers have been studied [1,15] such as support vector machine (SVM), minimax probability machine (MPM), fuzzy neighborhood discriminant analysis (FNDA), k-nearest neighbors (KNN), multilayer perceptron (MLP), self-organized map (SOM), radial basis function (RBF), regulatory feedback networks (RFN), hidden Markov model (HMM), and linear discriminant analysis (LDA). While traditional EMG controllers that use advanced signal processing and pattern recognition appear promising for the recovery of some function in prosthetic hands, still neural control of these devices remains incomplete and unreliable.

Developers have used traditional EMG control systems in many prosthetic and assistive devices. Jang et al. used the EMG signal to control an electric-powered wheelchair [17]. They used root mean square of error and project it to get the state. Gui et al. used RBF classifier for EMG signals to control an exoskeleton [18]. Lyons et al. used linear discriminant analysis to control an upper limb prosthesis by EMG signals[19]. They used a feature vector that consists of mean absolute value, wavelength, number of zero crossings, and number of slope sign changes. Segil et al. used the root mean square of EMG signal with a vector summation algorithm to control the radial motion of a prosthetic hand [20].

Recent advancements in general-purpose graphics processing units (GPGPUs) [21-23] enable devices to run a large set of computations in parallel (real-time). Deep neural networks, especially convolutional neural networks (CNN), benefit from the resulting computation power. Hence, the state-of-the-art optimization methods quickly change from subsystem optimization to end-to-end optimization [24-26]. Image segmentation [27], object detection [28], speech recognition [29], natural language processing [30], playing Atari game [31], object manipulation [32], autonomous driving [33], lung disease detection [34], and financial asset trading [35] are some of the examples of the optimization paradigm shift.

Few studies have been published on application of deep learning for pattern recognition of EMG signals. Atzori et al. archived 70% accuracy by using time windows of 150 ms, preprocessing, and a convolutional neural networks [36]. Their datasets were obtained using 12 electrodes from a Delsys Trigno Wireless System, providing the raw sEMG signal at 2 kHz. These electrodes were fixed on the forearm using standard adhesive bands and a hypoallergenic elastic latex-free band. Eight electrodes were positioned around the forearm at the height of the radio humeral joint at a constant distance from each other; two electrodes were placed on the main activity spots of the flexor digitorum superficialis and of the extensor digitorum superficialis, two electrodes were also placed on the main activity spots of the biceps brachii and of the triceps brachii. Zhai et al. used a CNN consisting of a convolutional layer of and two dense layers [37]. Their CNN input is a spectrogram of EMG signal (i.e. 2D) with window time of 200 ms. Their CNN achieved 78% accuracy. Cote-Allard et al. used a low cost, 8-channel, dry-electrode, low-sampling rate (200 Hz) armband sensor [38]. The data in their

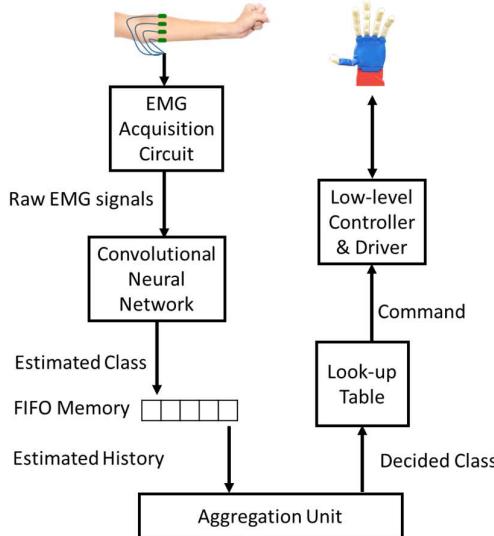


Fig. 2. Block diagram of the proposed method to control prosthetics hands with raw EMG signals using a convolutional neural network.

work, is separated by applying sliding windows of 260ms (to ensure sufficient time for data processing and classification) with an overlap of 235ms. For each of the eight channels of the armband, 52 samples (260ms) per spectrograms are leveraged using Hann windows of 28 points per fast Fourier transform (FFT) and an overlap of 20. This yields a matrix of 8x4x15 (Channels x Time bins x Frequency bins). Their proposed CNN has three convolutional layers and two dense layers. The few published works on deep learning of EMG signal are not complete. Further study is required for different sensor arrangements and CNN architecture. Also, new methods should be studied on CNN with raw EMG input (instead of spectrogram).

The main contribution of this paper is the development of a novel EMG based control system for prosthetics hand. The proposed system uses an array of 8 dry, linearly and evenly spaced EMG electrodes. We investigated many CNNs to find the optimal architecture for our sensor arrangement. The proposed convolutional neural networks directly uses raw EMG signals without any preprocessing, feature extraction, or spectrogram. The proposed method is a step toward a fully end-to-end optimization of EMG controlled prosthetic hands. Because the accuracy of the proposed CNN is not 100%, we propose a post-processing subsystem that includes a first input first output (FIFO) memory and an aggregation unit. The proposed post-processing subsystem will make our system error-free while adding a small delay.

This paper is organized as follows. Section II explains the proposed method for EMG-based control of prosthetic hand using deep convolutional neural networks. Section III presents the experimental results of the proposed method when implemented on an embedded GPGPU for prosthetic hands. Section IV explains a preliminary design of electrical circuits. Section V discusses the final products. The last section is a conclusion on the proposed EMG control of prosthetic hands.

II. METHOD

In this section, we describe a novel method to control prosthetic hands with EMG signals in detail. The main difference between the proposed method and traditional EMG

control systems is that instead of four subsystems of pre-processing, feature extraction, dimension reduction (feature description), and a classifier, we use only a novel convolutional neural network. Our novel convolutional neural network uses raw EMG data as input. Fig. 2 shows the block diagram of the system that consists of a novel convolutional neural network, a FIFO memory, an aggregation unit, and a look-up table.

In a study, researchers found that with proper signal processing techniques and pattern recognition systems, the accuracy from signals that captured from non-targeted muscles is close to the accuracy when sensors are exactly positioned above the targeted muscle [39]. Therefore, we decided to use data obtained from an array of eight linearly spaced sensors without concerning about their positioning relative to the muscle groups. While each sensor of this setup captures signals from multiple muscles simultaneously, it is a lot more convenient and simple to set up in repeated uses for amputees.

We decided to develop a novel end-to-end network for estimating the hand gesture class directly from raw EMG signals. The proposed convolutional neural network is novel because, we do not use any pre-processing subsystem and spectrograms. Here, we used 1D convolutional layers instead of 2D convolutional layers. The other novelty of the proposed CNN is that the filter sizes consistently decrease in deeper layers (not fixed). In this paper, we have access to a limited number of datasets such that we are not able to train very deep neural networks (more than 10 layers). As shown in Fig. 3, the proposed networks consist of 6 convolutional layers and 2 dense layers. The input of the networks is 8 vectors, with each vector consisting of 200 elements. The number 200 is the number of sampled data points when the sliding window is 0.1 s and the sampling rate is 2000 samples per second. In this method, we used one-hot encoding. Thus, the output of the network is a vector with number of element equal to the number of class (for example 15 for data set that we used) and the activation function of the last layer is SoftMax. The detail of the networks is stated in Table I.

We proposed to add a post-processing subsystem to overcome the remaining error caused by convolutional neural networks. This subsystem includes first input first output (FIFO) memory that holds the last estimated classes of the CNN and an aggregation unit. The size of FIFO is independent of the hardware (prosthetic hand) that were used. The size of FIFO depends only on the accuracy of the CNN. If someone finds a better CNN that does not have any error, the FIFO memory should be deleted, i.e. size of FIFO will be 1. Size of FIFO should be an odd number. The speed of prosthetic hand decreased linearly by increasing the size of the FIFO memory. Therefore, based on the trained CNN, we should find the minimum odd number such that for all hand gesture in the dataset, the aggregation of all elements in FIFO memory be constant over time when the hand gesture is constant. The CNN output from a stream of EMG signals is independent and identically distributed (iid). Let's denote the probability of misclassification of the CNN with ρ and the size of FIFO memory with n . The probability of misclassification after post-processing can be find with $\rho^{\frac{n+1}{2}}$. For example, if the probability of CNN misclassification is 0.1, the probabilities of misclassification after post-processing for FIFO memories with size of 1, 3, and 5 are 0.1, 0.01, 0.001, respectively. Here, we used a FIFO memory with size of 5. As shown in Fig. 4,

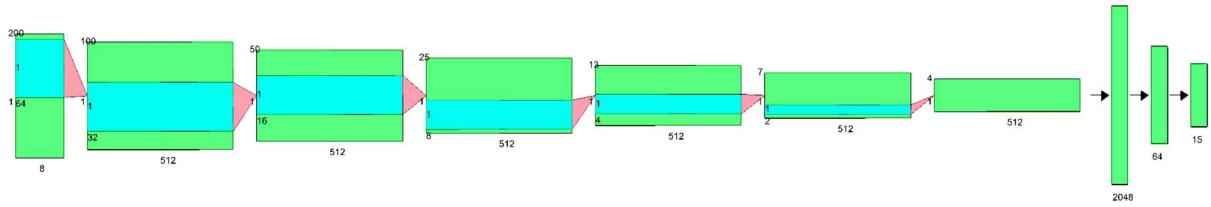


Fig. 3. Block diagram of the proposed convolutional neural network.

TABLE I. DATAILS OF THE PROPOSED CONVOLUTIONAL NEURAL NETWORK.

Layer	Type	Number of filters	Filter size	Stride	Activation	Output shape	Number of Parameters
0	Input (Raw EMG)	-	-	-	-	200 x 8	0
1	Convolution 1D	512	64	2	ReLU	100 x 512	262656
2	Convolution 1D	512	32	2	ReLU	50 x 512	8389120
3	Convolution 1D	512	16	2	ReLU	25 x 512	4194816
4	Convolution 1D	512	8	2	ReLU	13 x 512	2097664
5	Convolution 1D	512	4	2	ReLU	7 x 512	1049088
6	Convolution 1D	512	2	2	ReLU	4 x 512	524800
-	Flatten	-	-	-	-	2048	0
-	Drop out	-	-	-	-	2048	0
7	Dense	-	-	-	ReLU	64	131136
-	Drop out	-	-	-	-	64	0
8	Dense	-	-	-	SoftMax	15	975

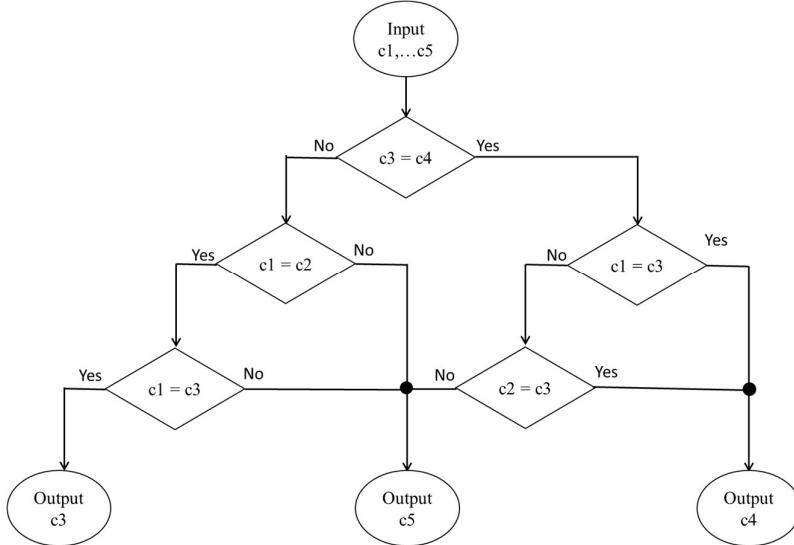


Fig. 4. Flowchart of the proposed aggregation unit for a FIFO memory with size of 5. The c_1, \dots, c_5 are predicted classes corresponding to latest CNN outputs.

the aggregation unit outputs the class that repeated more than half of the size of FIFO. For example for a FIFO with size of 5, output of aggregation unit is a class that repeated 3 times or more. If there is not a class with repetitions more than half of the size of the FIFO memory (here, 3), the output of aggregation unit is the latest estimated class. We used a look-up table to map the decided class (output of the aggregation unit) to a command for the low-level controller of prosthetic hand.

III. RESULTS

Selecting EMG dataset is the first steps of doing experiments. We used a dataset consisting 8 subjects, with 3 repetition (20 s long each) of 15 hand positions (total 45 data for each subject). The detail of dataset is stated in the Appendix. We chose this dataset because it uses the proposed

sensor arrangements (8 dry, linearly and evenly spaced) and data collected at a higher frequency (4000 sample per second). Then, We down-sampled the data to 2000 sample per second by jumping (not preprocessing). Selecting a high-performance GPGPU for training the networks is the second steps. We chose NVIDIA Tesla V100 GPGPU for our training. Therefore, we used V100 compute nodes in the Maverick2 at the Texas Advanced Computing Center (TACC), The University of Texas at Austin, Austin, TX, USA. A summary of the nodes specification are stated in Table II. The third step to experiment the proposed method is selecting an appropriate developer kit. There are few GPGPU developer kits available in the market that provide GPIO, UART, I2C, and SPI buses which are required to communicate with the devices that drive the prosthetic hands. Table III shows a comparison of the two most powerful GPGPU developer kits in the market.

TABLE II. MAVERICK2 V100 COMPUTE NODE SPECIFICATIONS

Rack	Dell PowerEdge R740
Processors	2 x Xeon(R) Platinum 8160 CPU 2.10GHz
GPGPUs	2 x NVidia Tesla V100
RAM	192 GB
Cores per processor	24
Total cores per node	48
Hardware threads per node	96
Local storage	119.5 GB (~32 GB free)

TABLE III. PROPOSED GPGPU DEVELOPER KITS

Company	NVIDIA	NVIDIA
Model	Jetson TX2	AGX Xavier
GPGPU	Pascal 256 core	Volta 512 core
TPU	-	-
CPU	4 core Cortex-A57 + 2 core Denver	8 core Camel
RAM	8 GB	16 GB
Storage	32 GB	32 GB
GFLOPS	559	1300
GPIO	8	4
USB	1 x USB 3.0 + 1 x USB 2.0	2 x USB C [3.1]
UART	1	1
I2C	4	2
SPI	1 with 2 CS	1 with 2 CS
CAN	1	1
I2S	2	1
Size (mm)	170 x 170 x 51	105 x 105 x 85
Weight	1.5 Kg	630g
Price (\$)	400	700

NVIDIA AGX Xavier developer kit is the best kit in the market (2019). However, we selected the NVIDIA Jetson TX2 because it provides enough computation power at a lower cost. These two boards are compatible such that users can replace NVIDIA Jetson TX2 with NVIDIA AGX Xavier easily.

The proposed convolutional neural network was implemented in Python 3.5 using the TensorFlow library. We used data from two subjects for testing and other subjects for training and validation. Out of the 3 repetitions of each movement, 2 were chosen and placed into the training set, the other repetition was placed in the validation set. Then all the 3 repetitions from the other 2 individuals were placed into the test set. The input of the proposed CNN is EMG measurement for 100 ms time window. The window slides every 10 ms. Each hand gesture collection was recorded for 20 s. Thus, the total number of time window in each record is 1991 ($1 + 20 - 0.1$). Therefore, the whole data consists of 358380 ($6 \times 15_{0.01} \times 2 \times 1991$) windows for training, 179190 windows ($6 \times 15 \times 1 \times 1991$) for validation and, 179190 ($2 \times 15 \times 3 \times 1991$) windows for testing. We have tried many different architectures of CNN. In our experiments, the eight-layer network (six convolutional layers and two dense layers) shows a validation accuracy of 91.26% (for training accuracy 99.98%). The test accuracy reaches to 48.40%. The training accuracy can be increased by using deeper networks. However, deeper networks result in lower validation accuracies. This is because we used a limited amount of data. We can conclude that by collecting more data and using a deeper network we can achieve better networks.

The results of the training, validation, and test accuracy of the proposed networks is demonstrated in Fig. 5. This CNN has 16,650,255 trainable parameters. The training of this CNN takes 10 hours (200 epochs) in the V100 compute node of Maverick2 supercomputer when the batch size is 4096 and

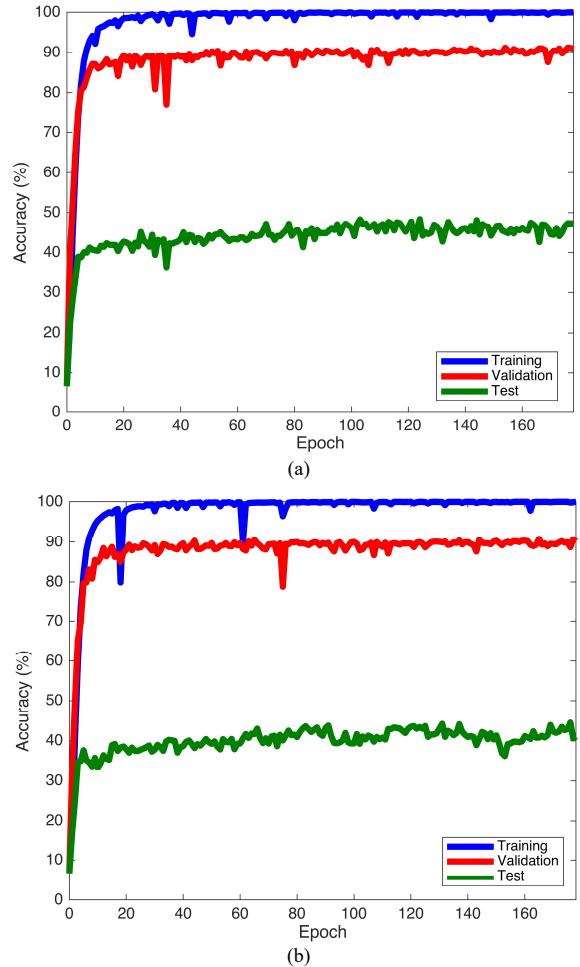


Fig. 5. Trend of accuracy of the proposed convolutional neural network for two sets of cross-validation (cross-testing).

TABLE IV. A COMPARISON BETWEEN THE PROPOSED CONVOLUTIONAL NEURAL NETWORKS AND OTHERS

Method	# sensors	Length (ms)	Input	Accuracy
Atzori et al. [36]	12	150	Preprocessed	70%
Zhai et al. [37]	12	200	Spectrogram	78%
Cote-Allard et al. [38]	8	260	Spectrogram	97.81
Proposed CNN	8	100	Raw	91.26%

optimizer is Adam (learning rate 0.0001, $\beta_1=0.9$, $\beta_2=0.999$, epsilon=1e-08). The test accuracy is low(48.40%). The main reason for the low test accuracy is the low amount of training data. Nevertheless, the proposed method can be used by fine-tuning of the networks for each new user. Table IV shows a comparison between the proposed CNN and others.

After training/validating/testing the proposed convolutional neural networks on the supercomputer, we transfer the trained CNN to the embedded GPGPU developer kit (NVIDIA Jetson TX2) for testing. The proposed convolutional neural networks run in real-time. The window slides in 100 ms to match with the desired speed for prosthetic hand low-level controller (10 Hz closed-loop control). We observed that signals are not misclassified in more than two connected windows in each stream by only the CNN, i.e.

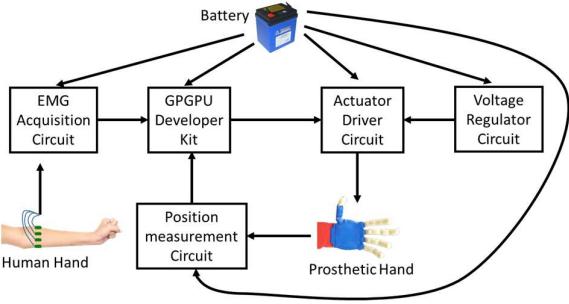


Fig. 6. Hardware diagram of the proposed method for EMG control of a prosthetic hand.

without the post-processing (FIFO memory and aggregation unit). In other words, the joint probability of three consecutive incorrectly estimated classes (CNN without the post-processing) is zero. Therefore, the proposed post-processing makes the final product error-free (functional).

IV. HARDWARE

The hardware of the proposed method consists five subsystems (Fig. 6): EMG acquisition circuit, GPGPU developer kit, actuator driver circuit, position measurement circuit, and voltage regulator circuit. The GPGPU developer kit can be either NVIDIA Jetson TX2 (cost efficient) or NVIDIA AGX Xavier (size efficient and faster). Both EMG acquisition circuit and position measurement circuit have eight 16-bit precision Sigma-Delta analog to digital converters (ADC) with a sampling rate of 2000 samples/second and an ultra-low noise and a low dropout 3.3V linear voltage regulator. To reduce the power input noise, we used a low-pass double LC filter in the both boards. The EMG acquisition circuit uses 8 instrumentation amplifiers (In Amp) with a gain of 660. The position measurement circuit uses 8 single-supply (output rail-to-rail) operation amplifiers in the buffer mode (gain 1) to read flex sensors (bending sensitive resistors). These two boards and the actuator board communicate with GPGPU developer kit via standard I2C bus. We decided to use a separate voltage regulator board for the actuators to have more modularity, thus allowing it to be adapted to a wide range of actuators. The actuator board consists of an 8-channel 16-bit digital to analog converter (DAC), 8 single-supply (output rail-to-rail) operation amplifiers (Op Amp), and 8 NPN bipolar junction transistors (BJT). The actuator board in tandem with regulator boards can provide up to 16V and 2.5 A in each channel, for up to 8 channel). The input power of each channel is independent and can be adjusted for different types of actuators. When the maximum voltage of the actuator is less than 4V, the voltage can be adjusted in the software (hardware adjusted to 4V). In this case the resolution of driver accuracy will drop linearly. For example, 1V actuator can be used with 14-bit accuracy. This resolution is enough for any prosthetic hands. The voltage regulator circuit consists of an adjustable low dropout linear voltage regulator and a double LC filter.

We used through hole components for the first prototype. However, in the future, we will use surface mount components to reduce noise and overall size. Fig. 7 shows schematics of instrumentation amplifier for the EMG signal, buffer for flex sensor (sensitive resistive), and power amplifier for actuator. Summary of the proposed components is stated in Table V.

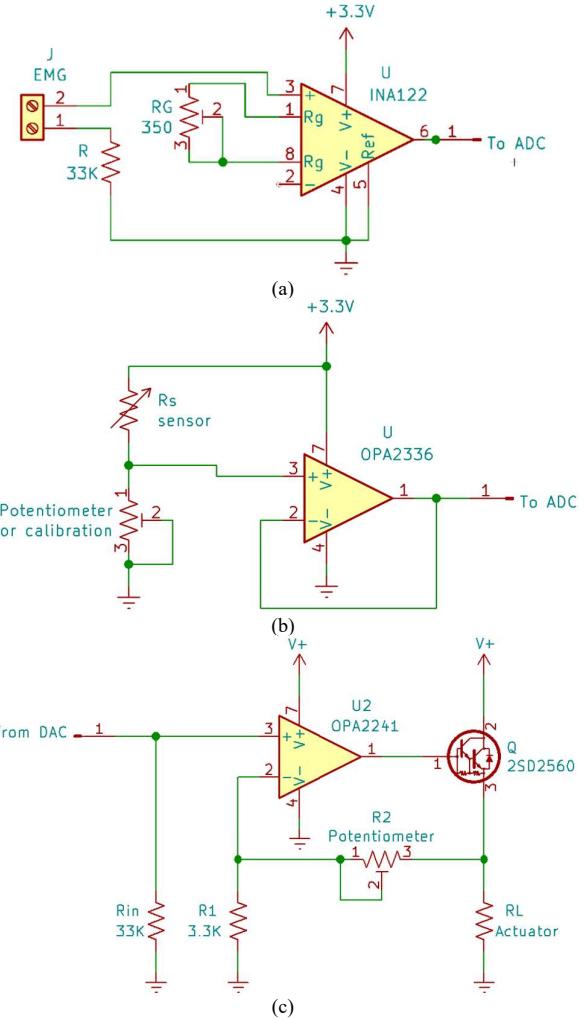


Fig. 7. Schematics of circuit (a) instrumentation amplifier for EMG signal (b) buffer for resistive sensor (such as flex sensor) (c) power amplifier for actuator.

TABLE V. SUMMARY OF PROPOSED COMPONENTS FOR FIRST PROTOTYPE

Components	Model	Description
DAC	LTC2605IGN-1#PBF	16-bit, I2C, 8 channels
ADC	TI ADS112C04IPWR	16-bit, I2C, Sigma-Delta, 2000 sample per second
I2C Isolator	TI ISO1540QDQ1	1Mbps 25kV/ μ s
In Amp	TI INA122	Single-Supply, rail-to-rail output, low noise 60nV/ \sqrt Hz
Op Amp	TI OPA 2336	Single-Supply (2.3V to 5.5V), rail-to-rail output (2 mV)
Op Amp	TI OPA2241	Single-Supply (2.7V to 36V), rail-to-rail output (50 mV)
BJT	Sanken 2SD2560	NPN, DC Current Gain 5000, Power Max 130W
Adjustable linear voltage regulator	LT1764AET#06PBF	Output 3A, dropout 0.34V, low noise 40 μ VRMS
3.3 V linear voltage regulator	TI LM1085IT-3.3/NOPB	load regulation 0.1%, 3A, low noise 38 μ VRMS

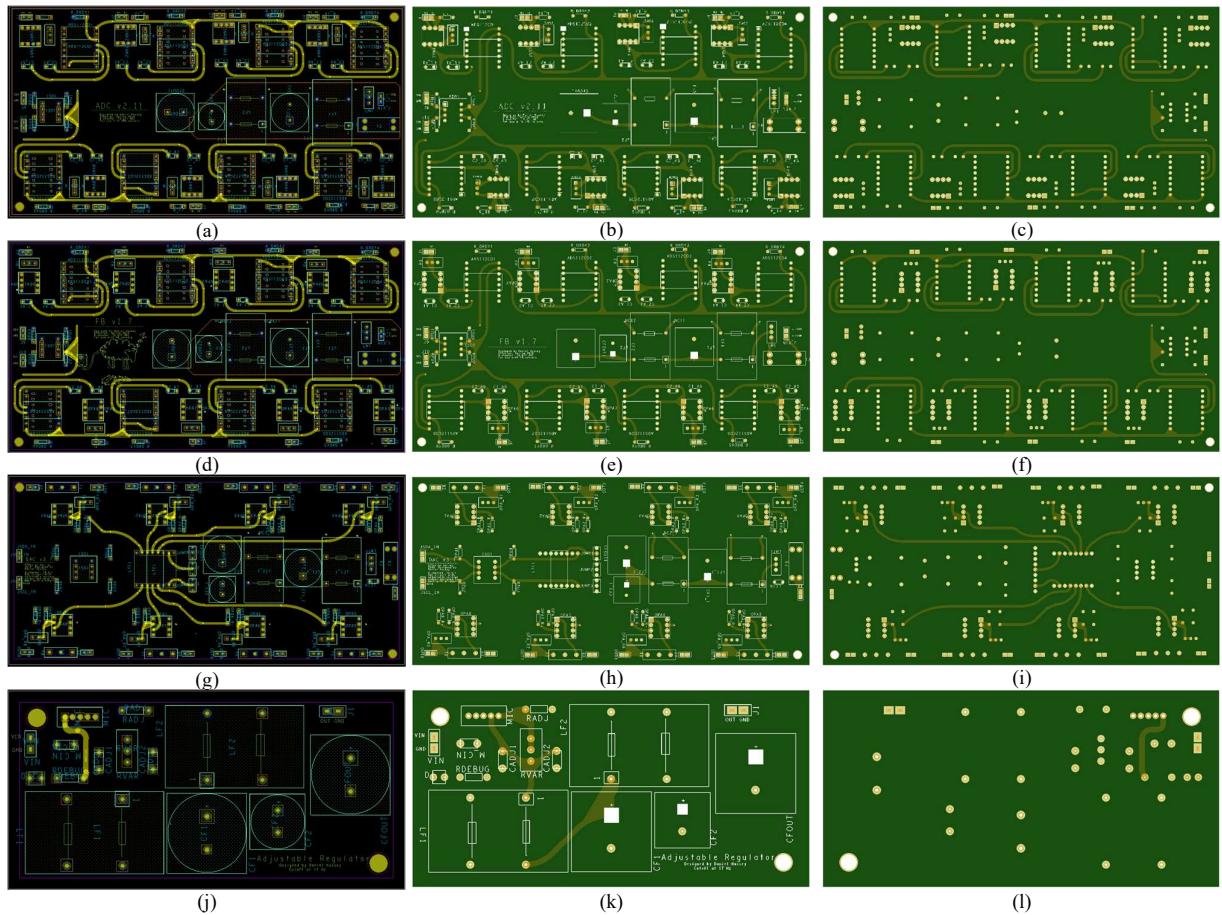


Fig.8. First prototype (a) EMG acquisition circuit CAD model (b) EMG acquisition circuit PCB front (c) EMG acquisition circuit PCB backside (d) position measurement circuit CAD model (e) position measurement circuit PCB front (f) position measurement circuit PCB backside (g) actuator driver circuit CAD model (h) actuator driver circuit PCB front (i) actuator driver circuit PCB backside (j) voltage regulator circuit CAD model (k) voltage regulator circuit PCB front (l) voltage regulator circuit PCB backside.

The CAD model and PCB of the first prototypes are illustrated in Fig. 8. The PCBs have been designed to be fabricated in green color, 2.0 mm thickness, 2 oz copper weight, and ENIG-RoHS surface finish.

V. DISCUSSIONS

In this paper, we used EMG data from 6 people for training/validation and two people for testing of the proposed network. The small gap between the training accuracy and the validation accuracy (Fig.5) shows that the proposed method is reliable (functional) when this CNN is fine-tuned for a specific person. However, there is a huge gap between the validation accuracy and the test accuracy. This large magnitude shows that the proposed method cannot be generalized to work for many different individuals. The first step in the future is increasing the number of people in the dataset from 8 to 100 or more in order to study the robustness (test accuracy). Another step will be investigating very deep convolutional neural network, which requires increasing the number of people to 1000 or even higher.

Here, we proposed the aggregation unit to overcome the small amount of the error in validation. The alternative way to the proposed post-processing subsystem is using a recurrent layer such as long short-term memory (LSTM) and gated recurrent unit (GRU). The recurrent neural networks consider

feedback from past decisions. However, the resulting networks require a higher amount of data. Thus, we will study these types of networks after collecting more data.

In this study, we used only the supervised classification learning method for application in prosthetic hands. The main disadvantage of the proposed method is that it is limited to a set of predefined positions (here 15 gestures). Imitation learning and reinforcement learning are other types of the learnings that can be used for continuous control of the hand (not a discrete finite set of predefined gesture). In the future, after collecting more data, we will study imitation learning and reinforcement learning technique for continuous control of prosthetic hands.

In this research, we focused on a method of controlling prosthetic hands using raw EMG signal as an input with deep convolutional neural networks. However, our methods can be implemented on the other prosthetic devices. The only difference is optimizing the architecture (layers) of convolutional neural networks for those particular devices. The only change will be update the mapping subsystem (look-up table).

VI. CONCLUSIONS

In this paper, we use deep learning techniques to develop a novel EMG based control system for prosthetics hands with

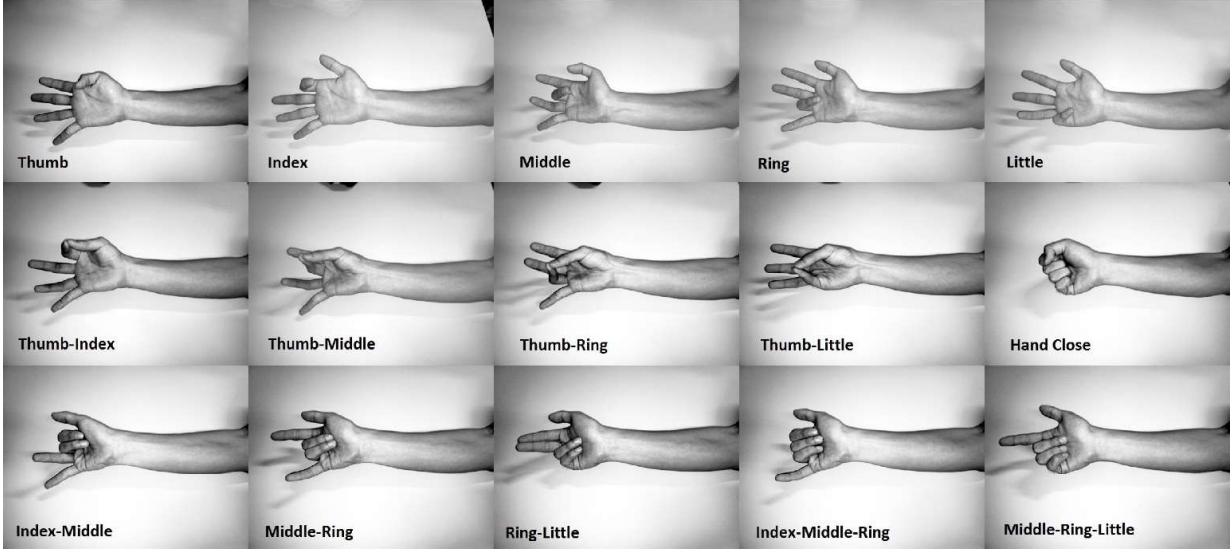


Fig. 10. Different classes of individual and combined fingers movement [40].

an array of 8 dry, linearly and evenly spaced surface EMG electrodes (2000 sample per second). In contrast to recent literature, the proposed convolutional neural network uses raw EMG (with window time of 0.1s) without any preprocessing (including a spectrogram). The proposed method was implemented in Python using the TensorFlow library. We use an NVIDIA Jetson TX2 developer kit (an embedded GPGPU board) to test the proposed methods.

We used a dataset that was obtained from 8 people with 15 hand gestures and 3 repetitions. Two of the three repetitions from 6 people are used for training, the third repetitions of 6 people are used for validation. All the signals from the other two persons were used for testing. The validation accuracy of the proposed method is 91.26%. Because the accuracy of the proposed convolutional neural network is not 100%, we propose a post-processing subsystem that includes a first input first output (FIFO) memory and an aggregation unit. The proposed post-processing subsystem makes our system error-free.

In the future, first, we will collect more EMG data from many people. After that, we will be able to study deeper neural networks. The low-test accuracy (48.40%) can be addressed by a higher amount of data. Then, we will compare recurrent neural networks with the proposed post-processing subsystem. The main disadvantage of the proposed method is that it is limited to a finite number of hand gestures (here 15). In the future, we will study deep imitation learning and deep reinforcement learning to address continues control of prosthetic hands with EMG signals.

APPENDIX: DATASET

Data is the most important part of any machine learning algorithm, especially deep learning. The proposed method uses an array of 8 EMG electrodes and raw EMG data for the neural network. We used the data set that was published by Khushaba and Kodagoda [40]. Here, we will explain how the data was recorded and the nature of the experiment as this data

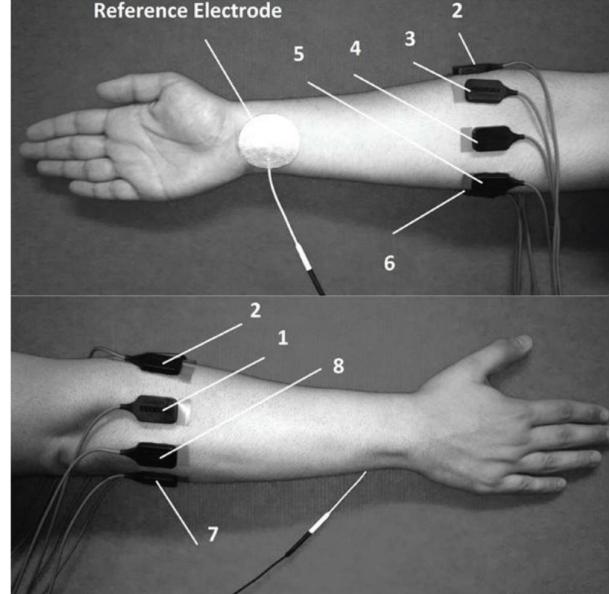


Fig. 9. EMG sensor arrangement [40].

is input to our network. In their project, eight subjects, six males and two females, aged between 20-35 years were recruited to perform the required fingers movements. The subjects were all able body subjects with no neurological or muscular disorders. Subjects were seated on an armchair, with their arm supported and fixed at one position. The datasets were recorded using eight EMG channels (DE 2.x series EMG sensors) mounted across the circumference of the forearm and processed by the Bagnoli desktop EMG system from Delsys Inc., as shown in Fig. 9. Fifteen classes of movements were collected including: the flexion of each of the individual fingers, i.e., Thumb, Index, Middle, Ring, Little and the combined Thumb-Index, Thumb-Middle, Thumb-Ring, Thumb-Little, Index-Middle, Middle-Ring, Ring-Little, Index-Middle-Ring, Middle-Ring-Little, and finally the hand close class as shown in Fig. 10. Subjects were asked to

TABLE VI. LOOK-UP TABLE FOR THE DATASET SHOWN IN FIG. 10.

Hand Gesture	Thumb Value	Index Value	Middle Value	Ring Value	Pinky Value
Thumb	1	0	0	0	0
Index	0	1	0	0	0
Middle	0	0	1	0	0
Ring	0	0	0	1	0
Little	0	0	0	0	1
Thumb-Index	1	1	0	0	0
Thumb-Middle	1	0	1	0	0
Thumb-Ring	1	0	0	1	0
Thumb-Little	1	0	0	0	1
Hand Close	0	0	0	0	0
Index-Middle	0	1	1	0	0
Middle-Ring	0	0	1	1	0
Ring-Little	0	0	0	1	1
Index-Middle-Ring	0	1	1	1	0
Middle-Ring-Little	0	0	1	1	1

perform 3 repetitions of the 15 different hand gestures. The data was captured with a rate of 4000 sample per second. We down-sampled to 2000 by jumping data points (not preprocessing). Fig. 11. Illustrates an input to the proposed convolutional neural network, which was a measurement result obtained from [40]. Table VI is the look-up table for this data set. The value (command) of a finger in the prosthetic hands is zero when the finger is fully relaxed. The value is one when the finger is fully contract.

ACKNOWLEDGMENT

We would like to thank Cameron Ovandipour and Ngoc Tuyet Nguyen Yount for valuable contributions in developing this project. We would like to express our very great appreciation to Dr. Marco Tacca, Dr. Nicholas Gans, Dr. Neal Skinner, and Dr. John Hanson, for comments and guidance that greatly improved the projects. We would also like to show our gratitude to Dr. Simmons and the Texas Advanced Computing Center (TACC), The University of Texas at Austin, Austin, TX, USA, for providing computational resources, (Maverick2 supercomputer).

REFERENCES

- [1] S. Micera, J. Carpaneto, and S. Raspopovic, "Control of Hand Prostheses Using Peripheral Information," IEEE Reviews in Biomedical Engineering, vol. 3, pp. 48–68, 2010.
- [2] K. Ziegler-Graham, E. J. MacKenzie, P. L. Ephraim, T. G. Travison, and R. Brookmeyer, "Estimating the prevalence of limb loss in the United States: 2005 to 2050," Arch Phys Med Rehabil, vol. 89, no. 3, pp. 422–429, Mar. 2008.
- [3] M. Marinoet al., "Access to prosthetic devices in developing countries: Pathways and challenges," in Proc. IEEE Annu. Global HumanitarianTechnol. Conf., 2015, pp. 45–51.
- [4] B. Maat, G. Smit, D. Plettenburg, P. Breedveld, "Passive prosthetic hands and tools: A literature review" Prosthet Orthot Int pp. 1-9 March 2017.
- [5] S. L. Carey, D. J. Lura, and M. J. Highsmith, "Differences in Myoelectric and Body-Powered Upper-Limb Prostheses," Journal of Prosthetics and Orthotics, vol. 29, no. 4s, pp. 4–20, 2017.
- [6] J. T. Kate, G. Smit, and P. Breedveld, "3D-printed upper limb prostheses: a review," Disability and Rehabilitation: Assistive Technology, vol. 12, no. 3, pp. 300–314, 2017.
- [7] C. Piazza, G. Grioli, M. Catalano, and A. Bicchi, "A Century of Robotic Hands," Annual Review of Control, Robotics, and Autonomous Systems, vol. 2, no. 1, pp. 1–32, 2019.
- [8] M. Controzzi, C. Cipriani, M. C. Carrozza, "Design of artificial hands: A review" in The Human Hand as an Inspiration for Robot Hand Develop USA NY New York:Springer pp. 219-246 2014.
- [9] D. Farina, N. Jiang, H. Rehbaum, A. Holobar, B. Graimann, H. Dietl, and O. C. Aszmann, "The Extraction of Neural Information from the Surface EMG for the Control of Upper-Limb Prostheses: Emerging Avenues and Challenges," IEEE Transactions on Neural Systems and Rehabilitation Engineering, vol. 22, no. 4, pp. 797–809, 2014.
- [10] L. H. Smith and L. J. Hargrove, "Comparison of surface and intramuscular EMG pattern recognition for simultaneous wrist/hand motion classification," 2013 35th Annual International Conference of the IEEE Engineering in Medicine and Biology Society (EMBC), 2013.
- [11] A. G. S. Rayo, L. H. H. Gómez, A. T. V. Sánchez, J. A. B. Fernández, J. A. F. Campos, G. U. Calderón, V. M. S. Rayo, and A. E. F. Peñaloza, "Design and Manufacturing of a Dry Electrode for EMG Signals Recording with Microneedles," Improved Performance of Materials Advanced Structured Materials, pp. 259–267, 2017.
- [12] M. Ergeneci, K. Gokcesu, E. Ertan, and P. Kosmas, "An Embedded, Eight Channel, Noise Canceling, Wireless, Wearable sEMG Data Acquisition System With Adaptive Muscle Contraction Detection," IEEE Transactions on Biomedical Circuits and Systems, vol. 12, no. 1, pp. 68–79, 2018.
- [13] M. Tomasini, S. Benatti, B. Milosevic, E. Farella, and L. Benini, "Power Line Interference Removal for High-Quality Continuous Biosignal Monitoring With Low-Power Wearable Devices," IEEE Sensors Journal, vol. 16, no. 10, pp. 3887–3895, 2016.
- [14] S. Benatti, F. Casamassima, B. Milosevic, E. Farella, P. Schonle, S. Fateh, T. Burger, Q. Huang, and L. Benini, "A Versatile Embedded Platform for EMG Acquisition and Gesture Recognition," IEEE Transactions on Biomedical Circuits and Systems, vol. 9, no. 5, pp. 620–630, 2015.
- [15] M. Simão, N. Mendes, O. Gibaru, and P. Neto, "A Review on Electromyography Decoding and Pattern Recognition for Human-Machine Interaction," IEEE Access, 2019.
- [16] M. G. Jahromi, H. Parsaei, A. Zamani, and D. W. Stashuk, "Cross Comparison of Motor Unit Potential Features Used in EMG Signal Decomposition," IEEE Transactions on Neural Systems and Rehabilitation Engineering, vol. 26, no. 5, pp. 1017–1025, 2018.
- [17] G. Jang, J. Kim, S. Lee, and Y. Choi, "EMG-based continuous control scheme with simple classifier for electric-powered wheelchair," IEEE Transactions on Industrial Electronics, vol. 63, no. 6, pp. 3695–3705, 2016.
- [18] K. Gui, H. Liu, and D. Zhang, "A Practical and Adaptive Method to Achieve EMG-based Torque Estimation for A Robotic Exoskeleton," IEEE/ASME Transactions on Mechatronics, 2019.
- [19] K. R. Lyons and S. S. Joshi, "Upper Limb Prosthesis Control for High-Level Amputees via Myoelectric Recognition of Leg Gestures," IEEE Transactions on Neural Systems and Rehabilitation Engineering, vol. 26, no. 5, pp. 1056–1066, 2018.
- [20] J. L. Segil and S. A. Huddle, "Functional assessment of a myoelectric postural controller and multi-functional prosthetic hand by persons with trans-radial limb loss," IEEE Transactions on Neural Systems and Rehabilitation Engineering, vol. 25, no. 6, pp. 618–627, 2017.
- [21] X. Shi et al. "Graph processing on GPUs: A survey" ACM Computing Surveys (CSUR) vol. 50 no. 6 pp. 81 2018.
- [22] S. Mittal, "A Survey on optimized implementation of deep learning models on the NVIDIA Jetson platform," Journal of Systems Architecture, 2019.

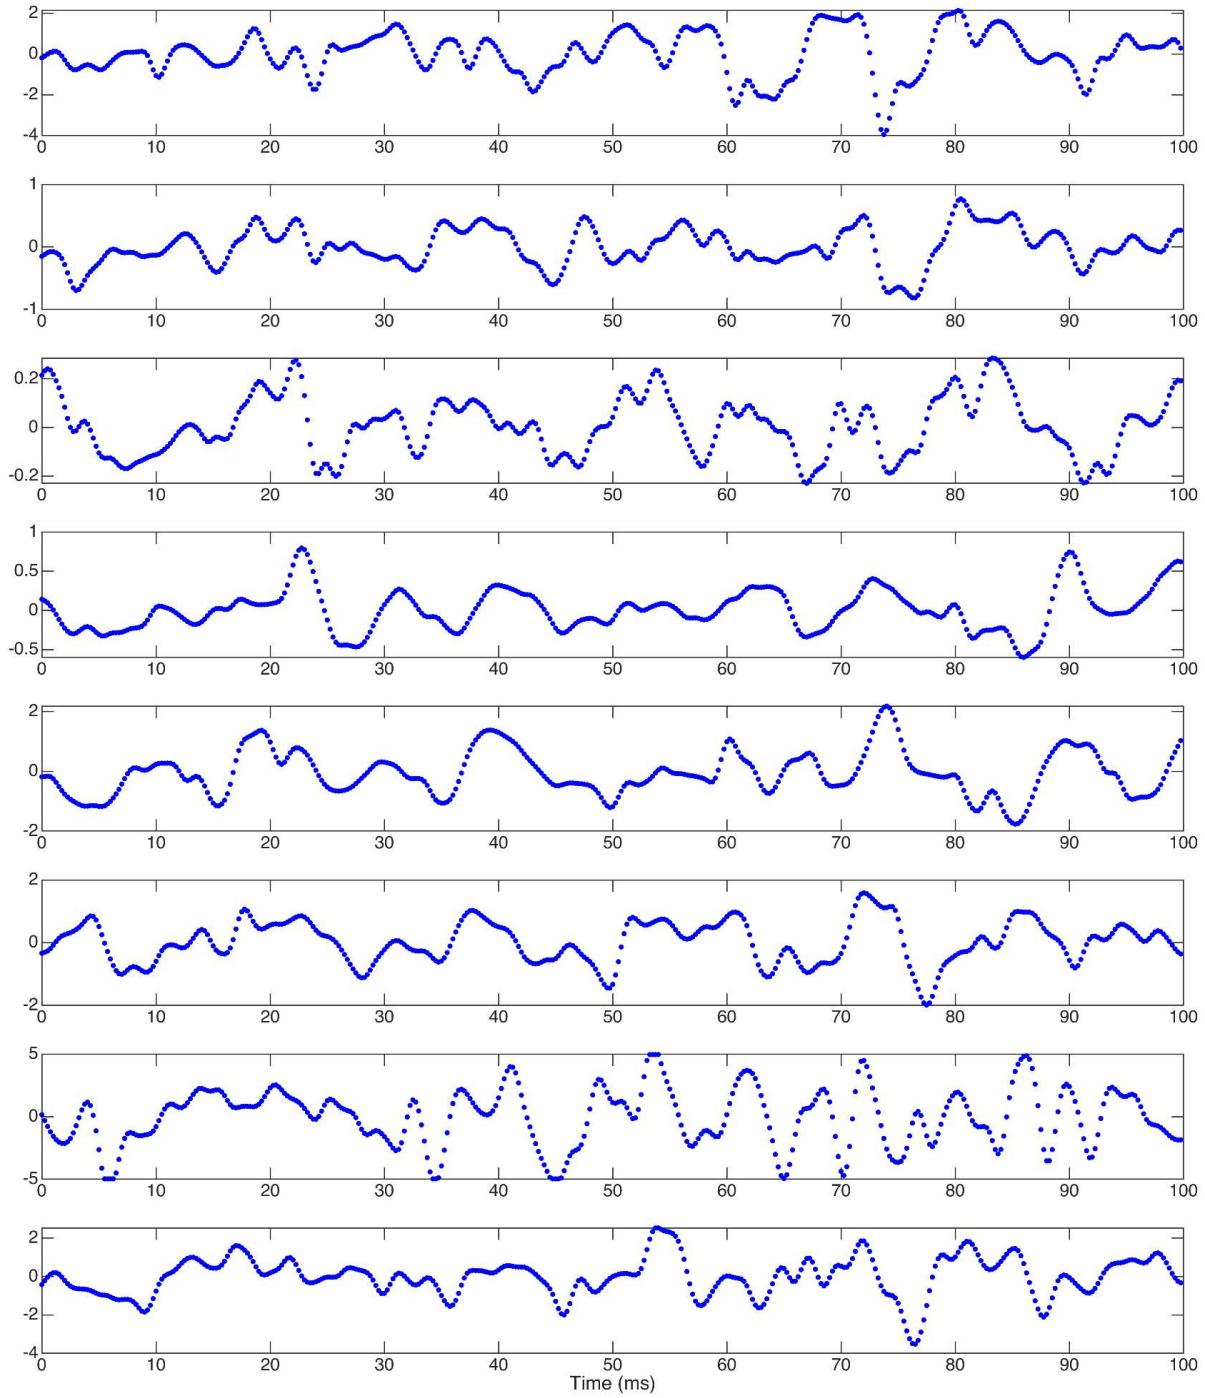


Fig. 11. Raw EMG signals obtained from human subject, which is one example of input data used in our convolutional neural network. The input data is in mV (raw EMG signals, 8 channels).

- [23] S. Migacz, "8-bit Inference with TensorRT," GPU Technology Conference, vol. 2, p. 7, 2017.
- [24] H.-C. Shin, H. R. Roth, M. Gao, L. Lu, Z. Xu, I. Nogues, J. Yao, D. Mollura, and R. M. Summers, "Deep Convolutional Neural Networks for Computer-Aided Detection: CNN Architectures, Dataset Characteristics and Transfer Learning," *IEEE Transactions on Medical Imaging*, vol. 35, no. 5, pp. 1285–1298, 2016.
- [25] Y. Lecun, Y. Bengio, and G. Hinton, "Deep learning," *Nature*, vol. 521, no. 7553, pp. 436–444, 2015.
- [26] J. Schmidhuber, "Deep learning in neural networks: An overview," *Neural Networks*, vol. 61, pp. 85–117, 2015.
- [27] V. Badrinarayanan, A. Kendall, and R. Cipolla, "SegNet: A Deep Convolutional Encoder-Decoder Architecture for Image Segmentation," *IEEE Transactions on Pattern Analysis and Machine Intelligence*, vol. 39, no. 12, pp. 2481–2495, 2017.
- [28] S. Zhang, L. Wen, X. Bian, Z. Lei, and S. Z. Li, "Single-Shot Refinement Neural Network for Object Detection," 2018 IEEE/CVF Conference on Computer Vision and Pattern Recognition, 2018.
- [29] T. Tan, Y. Qian, H. Hu, Y. Zhou, W. Ding, and K. Yu, "Adaptive very deep convolutional residual network for noise robust speech recognition," *IEEE/ACM Transactions on Audio, Speech, and Language Processing*, vol. 26, no. 8, pp. 1393–1405, 2018.

- [30] T. Young, D. Hazarika, S. Poria, and E. Cambria, "Recent Trends in Deep Learning Based Natural Language Processing [Review Article]," *IEEE Computational Intelligence Magazine*, vol. 13, no. 3, pp. 55–75, 2018.
- [31] V. Mnih, et al., "Human-level control through deep reinforcement learning," *Nature*, vol. 518, no. 7540, pp. 529–533, 2015.
- [32] S. Levine, P. Pastor, A. Krizhevsky, J. Ibarz, and D. Quillen, "Learning hand-eye coordination for robotic grasping with deep learning and large-scale data collection," *The International Journal of Robotics Research*, vol. 37, no. 4-5, pp. 421–436, 2017.
- [33] D. Li, D. Zhao, Q. Zhang, and Y. Chen, "Reinforcement Learning and Deep Learning Based Lateral Control for Autonomous Driving [Application Notes]," *IEEE Computational Intelligence Magazine*, vol. 14, no. 2, pp. 83–98, 2019.
- [34] H. C. Shin, et al., "Deep Convolutional Neural Networks for Computer-Aided Detection: CNN Architectures, Dataset Characteristics and Transfer Learning," *IEEE Transactions on Medical Imaging*, vol. 35, no. 5, pp. 1285–1298, 2016.
- [35] Y. Deng, F. Bao, Y. Kong, Z. Ren, and Q. Dai, "Deep Direct Reinforcement Learning for Financial Signal Representation and Trading," *IEEE Transactions on Neural Networks and Learning Systems*, vol. 28, no. 3, pp. 653–664, 2017.
- [36] M. Atzori, M. Cognolato, and H. Müller, "Deep Learning with Convolutional Neural Networks Applied to Electromyography Data: A Resource for the Classification of Movements for Prosthetic Hands," *Frontiers in Neurorobotics*, vol. 10, 2016.
- [37] X. Zhai, B. Jelfs, R. H. M. Chan, and C. Tin, "Self-Recalibrating Surface EMG Pattern Recognition for Neuroprosthesis Control Based on Convolutional Neural Network," *Frontiers in Neuroscience*, vol. 11, 2017.
- [38] U. Cote-Allard, C. L. Fall, A. Campeau-Lecours, C. Gosselin, F. Laviolette, and B. Gosselin, "Transfer learning for sEMG hand gestures recognition using convolutional neural networks," *2017 IEEE International Conference on Systems, Man, and Cybernetics (SMC)*, 2017.
- [39] T. Farrell and R. Weir, "A Comparison of the Effects of Electrode Implantation and Targeting on Pattern Classification Accuracy for Prostheses Control," *IEEE Transactions on Biomedical Engineering*, vol. 55, no. 9, pp. 2198–2211, 2008.
- [40] R. N. Khushaba and S. Kodagoda, "Electromyogram (EMG) feature reduction using Mutual Components Analysis for multifunction prosthetic fingers control," *2012 12th International Conference on Control Automation Robotics & Vision (ICARCV)*, 2012.

© 2019 IEEE. Personal use of this material is permitted. Permission from IEEE must be obtained for all other uses, in any current or future media, including reprinting/republishing this material for advertising or promotional purposes, creating new collective works, for resale or redistribution to servers or lists, or reuse of any copyrighted component of this work in other works.

IEEE

M. Jafarzadeh, D. Hussey and Y. Tadesse, "Deep learning approach to control of prosthetic hands with electromyography signals", in *2019 IEEE International Symposium on Measurement and Control in Robotics (ISMCR)*, Houston, Texas, USA, 2019.

ACM

Jafarzadeh, M., Hussey, D. and Tadesse, Y., 2019. Deep learning approach to control of prosthetic hands with electromyography signals. In *2019 IEEE International Symposium on Measurement and Control in Robotics (ISMCR)*. IEEE.

MLA

Jafarzadeh, Mohsen et al. "Deep Learning Approach To Control Of Prosthetic Hands With Electromyography Signals". IEEE, *2019 IEEE International Symposium On Measurement And Control In Robotics (ISMCR)*. IEEE, 2019.

APA

Jafarzadeh, M., Hussey, D., & Tadesse, Y. (2019). Deep learning approach to control of prosthetic hands with electromyography signals. In *2019 IEEE International Symposium on Measurement and Control in Robotics (ISMCR)*. Houston, Texas, USA: IEEE.

Harvard

Jafarzadeh, M., Hussey, D. and Tadesse, Y. (2019). Deep learning approach to control of prosthetic hands with electromyography signals. In: *2019 IEEE International Symposium on Measurement and Control in Robotics (ISMCR)*. IEEE.

Vancouver

Jafarzadeh M, Hussey D, Tadesse Y. Deep learning approach to control of prosthetic hands with electromyography signals. In: *2019 IEEE International Symposium on Measurement and Control in Robotics (ISMCR)*. IEEE; 2019.

Chicago

Jafarzadeh, Mohsen, Daniel Curtiss Hussey, and Yonas Tadesse. 2019. "Deep Learning Approach To Control Of Prosthetic Hands With Electromyography Signals". In *2019 IEEE International Symposium On Measurement And Control In Robotics (ISMCR)*. IEEE.

BibTeX

```
@inbook{ jafarzadeh_hussey_tadesse_2019,[break] title={Deep learning approach to control of prosthetic hands with electromyography signals},[break] booktitle={2019 IEEE International Symposium on Measurement and Control in Robotics (ISMCR)},[break] publisher={IEEE},[break] author={Jafarzadeh, Mohsen and Hussey, Daniel Curtiss and Tadesse, Yonas},[break] year={2019}}
```